T R A D I N G C O M P A N Y

SAFARINO BUSINESS CONSULTANT LIMITED



(北京中检安泰诊断科技有限公司)

Antai Diagnostic Technology Co., Ltd.

Dr.BASSAM SAFARINY

jo.no 00962791618420 china.no 0086-13632340078







Disposable Earloop Face Mask, Thick 3-Ply Medical Masks with Elastic Ear Loop, Breathable Non-woven

Dust Filter Face Mask, Breathable and Comfortable for Dust, (50PCS)







TRADING COMPANY





color avalabile gary and white



face mask



5 Medi-Inn Disposable Quality Visitors Lab

TRADING COMPANY







Coats Protective Non Woven Gown NEW

corona Test



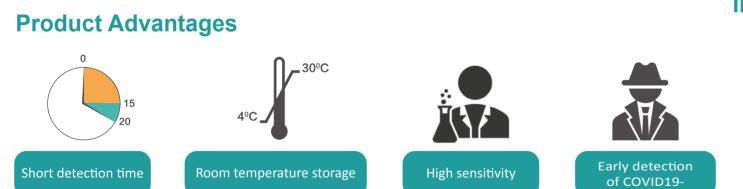


Instruction to Use

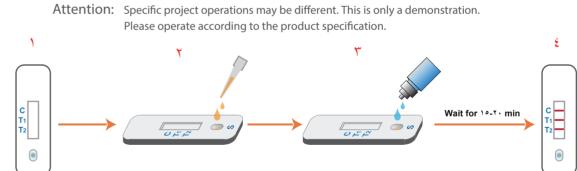




Add Y droplets of diluent

Interpretation of Results




Positive result. Indicates that the patient is infected by COVID¹⁹- in the early stage and the present stage.

Positive result. The patient may be currently infected or had previous infection. The final confirmation should be combined with clinical symptoms or with a molecular test.



Negative result. indicates that the patient is not infected by COVID19- or the level of antibody is too low to detect. Repeat the test again in a few days.



Product Performance The Rapid Test was tested in the Chinese Center for Disease Control and Prevention using samples from clinically confirmed patients.

IndexDetection rateCOVID۱۹-T۱٪۲۰٫۰COVID۱۹-T۲٪۹۳,۳T۱+T۲٪۱۰۰,۰Specificity٪۹۰,۲



SAFARINO BUSINESS CONSULTANT LIMITED

bipap@oxgyen

BiPAP& Oxygen Concentrator Combo Completely connects a CPAP and an oxygen

concentrator through the integrated structure and data protocol, providing a one-stop solution for patients who need CPAP & oxygen treatment, which greatly improve the conveniences, mobility and the effects of treatment.

Model: YC28

THOUGHTFULNESS

Provide integrated solution for patients in need of oxygen and CPAP treatment.

MOBILITY

One-stop structure enables easy mobility when using the CPAP and oxygen concentrator.

INTERACTION


O2 density and flux of the oxygen concentrator will be displayed with CPAP parameters on a 5" LCD screen.




DATA SHARING

Treatment data can be uploaded to an cellphone APP and a CLOUD platform in real time.





The chart shows how the integrated Respiratory Combo works. During the exhalation phase, when the oxygen concentrator receives a signal from the CPAP, it will reduces the oxygen concentration output and increases the oxygen concentration when the CPAP is in inhalation phase. It greatly improves the output efficiency of the oxygen concentrator and reduces energy consumption, which will be more environmentally friendly and economical.

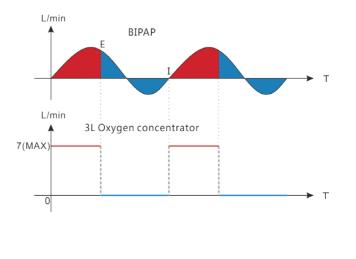





saftey clothes



Disposable Non-woven Fabric Protective Coveralls

Safety Clothing Isolation Gown For Hospitals







Disposable Non-woven Fabric Protective Coveralls

Safety cap Isolation Gown For Hospitals





Disposable Non-woven Fabric Protective Coveralls Safety shoes cover Isolation Gown For Hospitals






sterilizing gate









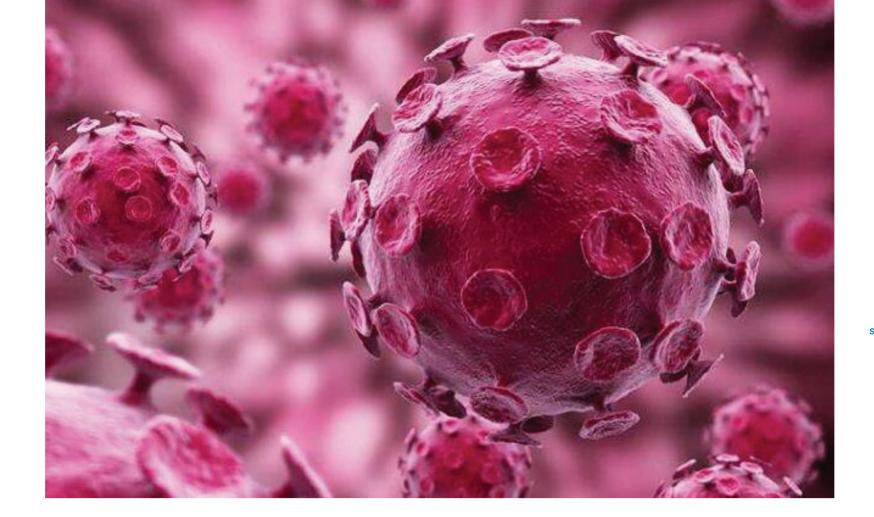

Corona Virus (COVID-19) Combined IgA/IgM/IgG Rapid Test

الدكتور بسام السفاريني

Dr.BASSAM SAFARINY 0086-13632340078 MSN: BASSAMNS@HOTMAIL.COM E-MAIL: ALSAFARINY@GMAIL.COM



(北京中检安泰诊断科技有限公司)

Antai Diagnostic Technology Co., Ltd.

